


Effectiveness - Predictability and accuracy of MRSE correction

(all eyes with successful SMILE treatment)

Predictability and accuracy of the MRSE correction is excellent across the entire range of attempted corrections.

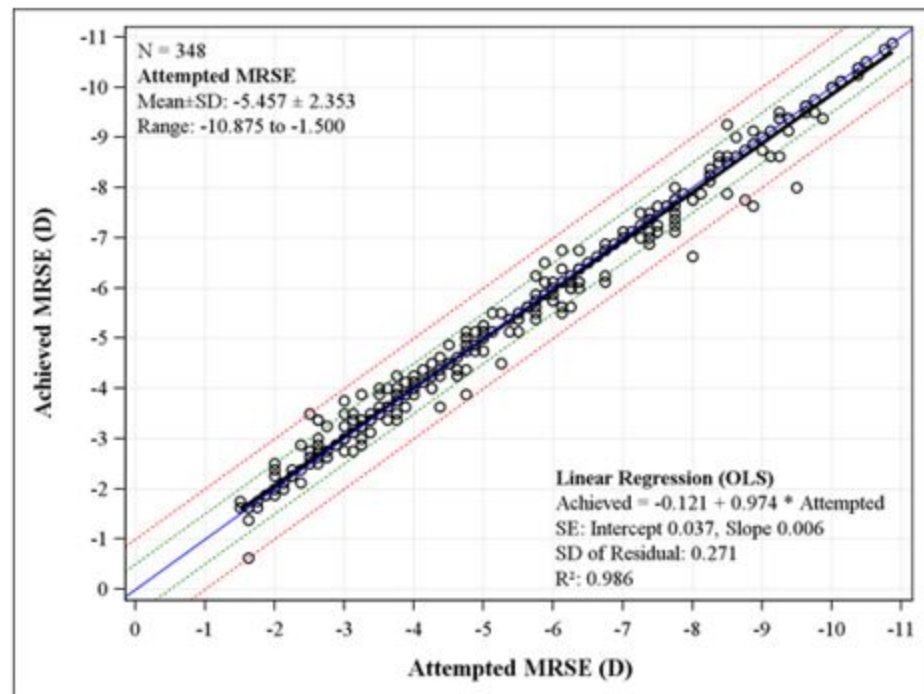

Mean attempted MRSE correction -5.44 D

at 6-month point of refractive stability:

Mean deviation from attempted MRSE correction -0.02 D

MRSE within

± 0.25 D 80% of eyes

± 0.50 D 93% of eyes

± 1.00 D 99 % of eyes